



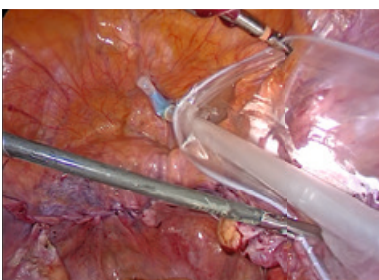

MetraBag
Controlled tissue morcellation
in an enclosed system

MetraBag

The FDA (U.S. Food and Drug Administration) recommends the use of a tissue containment system for morcellation during hysterectomy and myomectomy.

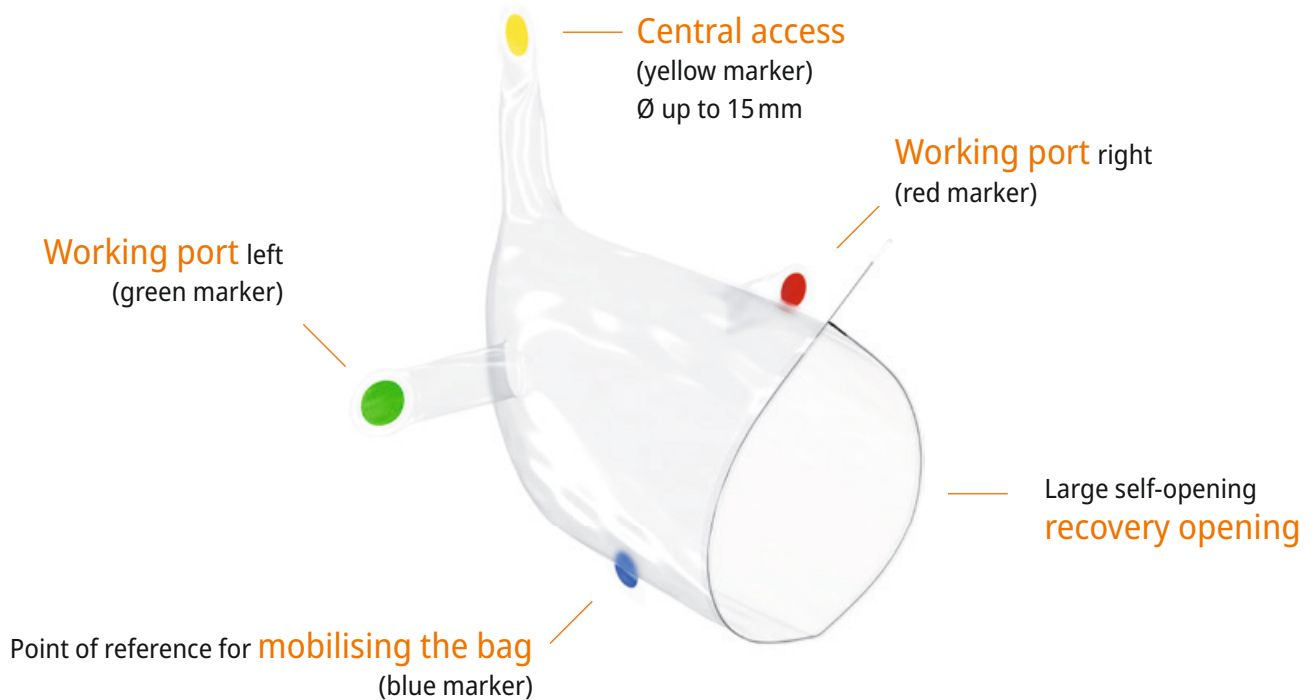

- MetraBag prevents residual tissue from being left behind in the abdomen without time-consuming suctioning.
- The variable working ports allow you to morcellate in a familiar way.
- The transparent MetraBag material provides a familiar working environment by maintaining visibility of surrounding structures.
- It is possible to introduce the MetraBag via a 10 mm trocar.



The MetraBag has been on the market for several years and has already been used in thousands of applications.



vimeo.com/774690588



Always up to date! MetraBag – Safety during Morcellation



www.ncbi.nlm.nih.gov/pmc/articles/PMC8536670/



M. Anapolski MD, Senior Consultant

Ordering information

	MetraBag	REF
	comprising: <ul style="list-style-type: none"> • Morcellation bag • Insertion aid • 3 drawstrings Sterile, 1 pack of ten	905-710

BOWA MEDICAL provides the tissue morcellation solution for your gynaecological procedures

Contact your authorised BOWA medical devices consultant now.

support@bowa-medical.com

BOWA
A C A D E M Y

EXPERTISE ensures SAFETY

Discover what the BOWA ACADEMY has to offer now



Online course and certificate



Checklist on HF surgery



bowa-medical.com/academy



Advanced training events



Live and on-demand webinars